


TEST REPORT

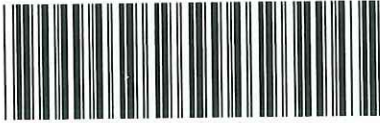

No: 210001071

VERIFICATION WEBSITE: www.gtt.net.cn

VERIFICATION CODE: CCVW-4032-14

DATE: 2021-07-29

APPLICANT: Guangzhou Powecom Labor Insurance Supplies Co., Ltd.
Floor 1, 3 and 4, Building 1, No. 43, Tuanjie Road, Xinya Street, Huadu District,
Guangzhou City, Guangdong Province, P. R. China

THIRTY(30) PIECES OF KN95 Protective Mask

BRAND: POWECOM

STYLE NO. : 202107

SIZE: KN95

DATE RECEIVED/DATE TEST STARTED: 2021-07-23 14:45

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
HEAD BAND	M

NOTE: "M" -MEET CLIENT'S REQUIREMENT "F" -BELOW CLIENT'S REQUIREMENT
"---" -NO COMMENT "N" -HALF GRADE LOW "L" -ONE GRADE LOW

REMARK:


IN THIS REPORT, THE SAMPLES ARE TESTED UNDER PRESCRIBED ENVIRONMENTAL CONDITIONS IN THE CORRESPONDING STANDARDS, UNLESS OTHERWISE NOTED.

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

WHEN THE INFORMATION PROVIDED BY THE CUSTOMER MAY AFFECT THE EFFECTIVENESS OF THE RESULTS, OUR INSTITUTE WILL NOT ASSUME ANY RESPONSIBILITY.

AUTHORIZED SIGNATORY:


WenLi Liu SENIOR ENGINEER



page 1 of 3

TEST REPORT

No:210001071

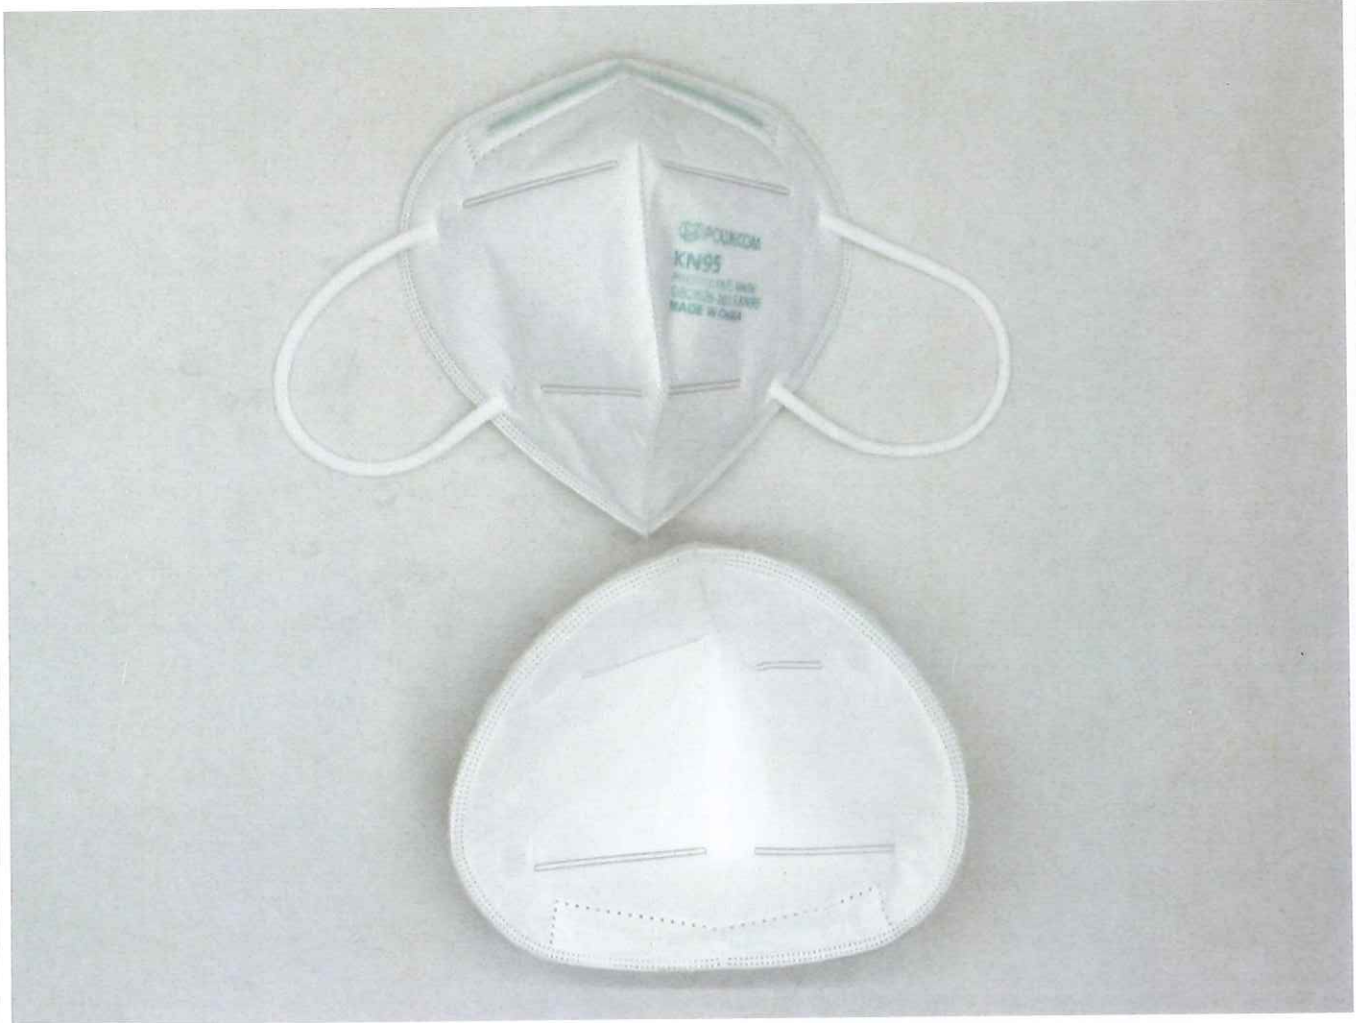

品检
专用章

TEST REPORT

No:210001071

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER (%)

(GB 2626-2019 6.3 AIR FLOW:85L/min AEROSOL:NaCl AEROSOL CONCENTRATION:15mg/m³
TEMPERATURE:25.5°C RH: 38.0%)

UNTREATED SAMPLE:

1# 99.70 2# 99.61
3# 99.66 4# 99.55
5# 99.71 6# 99.65
7# 99.60 8# 99.54
9# 99.64 10# 99.71
11# 99.64 12# 99.57
13# 99.54 14# 99.55
15# 99.64

REQUIREMENT

≥95.0
(KN95)
(GB 2626-2019)

SAMPLE AFTER PRETREATMENT:

1# 99.47 2# 99.37
3# 99.40 4# 99.49
5# 99.52

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2019 6.5 HEAD MODEL:MEDIUM)

UNTREATED SAMPLE

1#: 94.5
2#: 100.4

SAMPLE AFTER PRETREATMENT

1#: 84.7
2#: 85.7

REQUIREMENT

≤210
(GB 2626-2019)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2019 6.6 HEAD MODEL:MEDIUM)

UNTREATED SAMPLE

1#: 77.6
2#: 79.3

SAMPLE AFTER PRETREATMENT

1#: 77.8
2#: 76.6

REQUIREMENT

≤210
(GB 2626-2019)

HEAD BAND

(GB 2626-2019 6.11)

PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST
PARTS OF MASK SHOULD NOT SLIP OR BREAK
UNDER 10N TENSION FOR 10S.
(DISPOSABLE MASK)
(GB 2626-2019)

